

Regenerative Research
Denver, CO 80210



Project 135643
Lab # 131732
Date Rec'd 12/27/2025
Report Issued 1/20/2026

Project

Sample GLOW 70 mg (GW26-01)

Certificate of Analysis



<u>Analyte</u>	<u>Result</u>	<u>LOQ</u>	<u>Units</u>	<u>% of Label</u>	<u>Method</u>	<u>Date</u>	<u>CAS</u>
Peptide Analysis							
Chromatographic purity	99.72	0.5	%		HPLC-UV/MS	1/15/2026	
BPC-157	10.0	0.5	mg	100.3	HPLC-UV-MS	1/15/2026	137525-51-0
BPC-157	ID Confirmed				HPLC-UV-MS	1/15/2026	
GHK-Cu	43.8	0.5	mg	87.6	HPLC-UV-MS	1/15/2026	49557-75-7
GHK-Cu	ID Confirmed				HPLC-UV-MS	1/15/2026	
Thymosin β 4	9.47	0.5	mg	94.7	HPLC-UV-MS	1/15/2026	77591-33-4
Thymosin β 4	ID Confirmed				HPLC-UV-MS	1/15/2026	
Microbiology							
Endotoxins	ND	1	EU/mL		USP 85	1/16/2026	

The data presented are from the analysis of the sample shown and meet Krause Analytical internal quality assurance criteria unless otherwise flagged.
Methods shown reference current Krause Analytical SOPs
ND - Not detected LOQ - limit of quantification
Copyright © 2025 Krause Analytical LLC. All rights reserved.


Respectfully submitted,

Mark C. Krause
Laboratory Director



Chromatogram

Response_

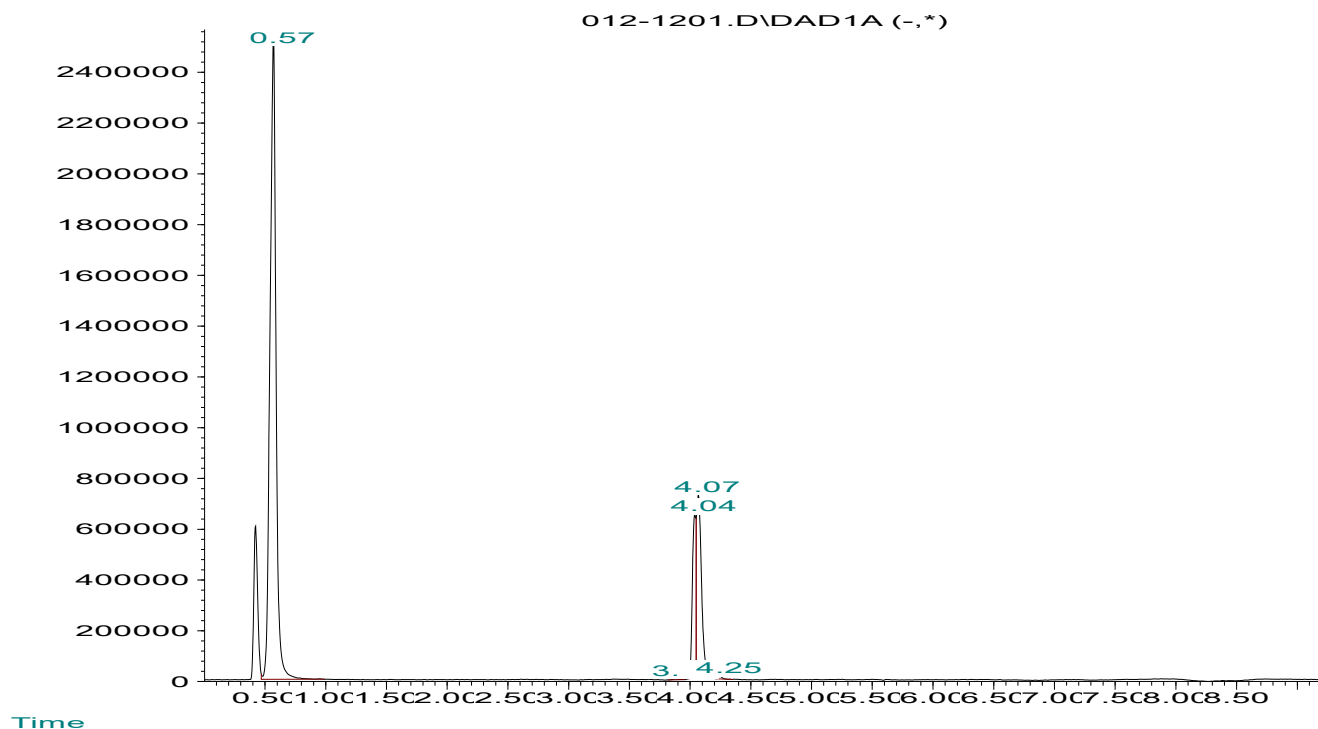

Mass spectrum/Reference Spectrum

