

Randy Cole
Regenerative Research
Denver, CO 80210



Project 135319
Lab # 128697
Date Rec'd 9/22/2025
Report Issued 10/8/2025

Project

Sample hCG 5000 iu HC25-01

Certificate of Analysis

Analyte

Microbiology

Endotoxins

Peptide Analysis

Chromatographic purity

Total peptide mass

Mass spectral identification

<u>Result</u>	<u>LOQ</u>	<u>Units</u>	<u>Method</u>	<u>Date</u>	<u>% of Label</u>
ND	1.0	EU/mL	USP 85	9/29/2025	
>99.95	0.5	%	HPLC-UV/MS	9/29/2025	
5,650	0.5	IU	HPLC-UV/MS	9/29/2025	112.9
Confirmed			HPLC-UV/MS	9/29/2025	

The data presented are from the analysis of the sample shown and meet Krause Analytical internal quality assurance criteria unless otherwise flagged.
Methods shown reference current Krause Analytical SOPs
ND - Not detected LOQ - limit of quantification
Copyright © 2025 Krause Analytical LLC. All rights reserved.

Respectfully submitted,


Mark C. Krause
Laboratory Director



krause analytical

Chromatogram

Response_

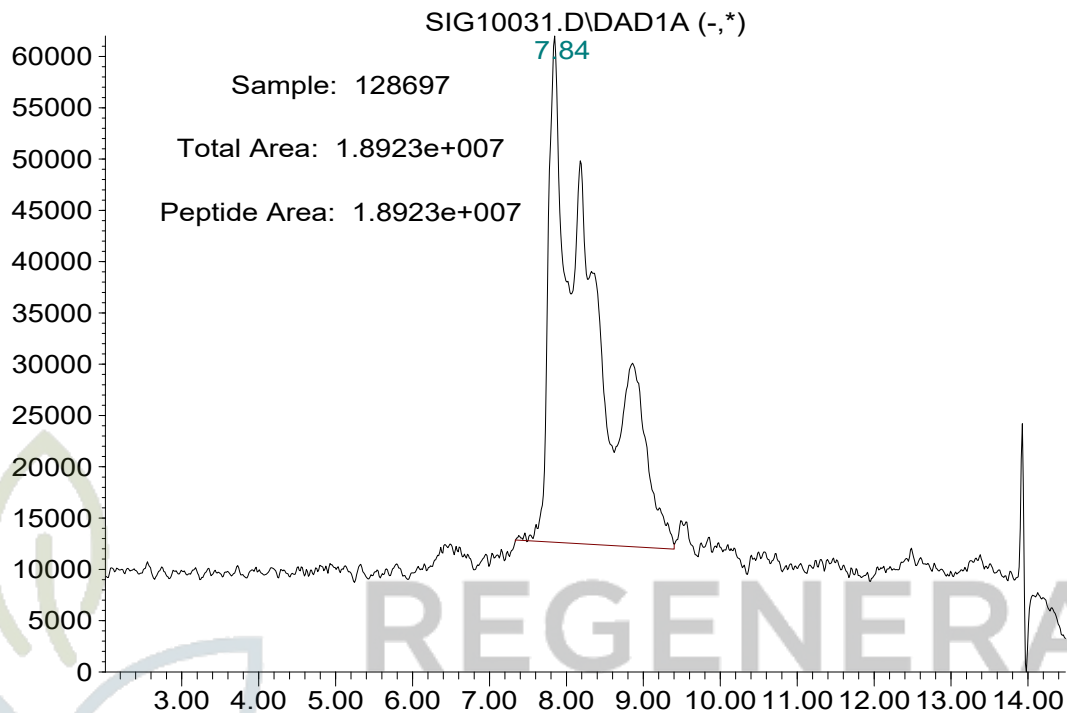

Mass spectrum/Reference Spectrum

