

Randy Cole
Regenerative Research
Denver, CO 80210




Project 135521
Lab # 130614
Date Rec'd 11/25/2025
Report Issued 12/1/2025

Project

Sample Retatrutide 10 mg (batch RT-25-06)

Certificate of Analysis

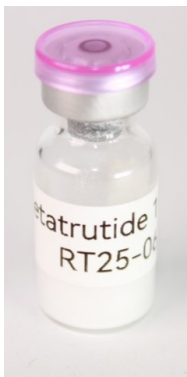**Analyte****Peptide Analysis**

Chromatographic purity

Retatrutide

Retatrutide

Microbiology

Endotoxins

<u>Result</u>	<u>LOQ</u>	<u>Units</u>	<u>% of Label</u>	<u>Method</u>	<u>Date</u>	<u>CAS</u>
>99.95	0.5	%		HPLC-UV/MS	11/28/2025	
10.4	0.5	mg	104.5	HPLC-UV-MS	11/28/2025	2381089-83-2
ID Confirmed				HPLC-UV-MS	11/28/2025	2381089-83-2
ND	1	EU/mL		USP 85	11/29/2025	

The data presented are from the analysis of the sample shown and meet Krause Analytical internal quality assurance criteria unless otherwise flagged.

Methods shown reference current Krause Analytical SOPs

ND - Not detected LOQ - limit of quantification

Copyright © 2025 Krause Analytical LLC. All rights reserved.


Respectfully submitted,

Mark C. Krause
Laboratory Director



Chromatogram

Response_

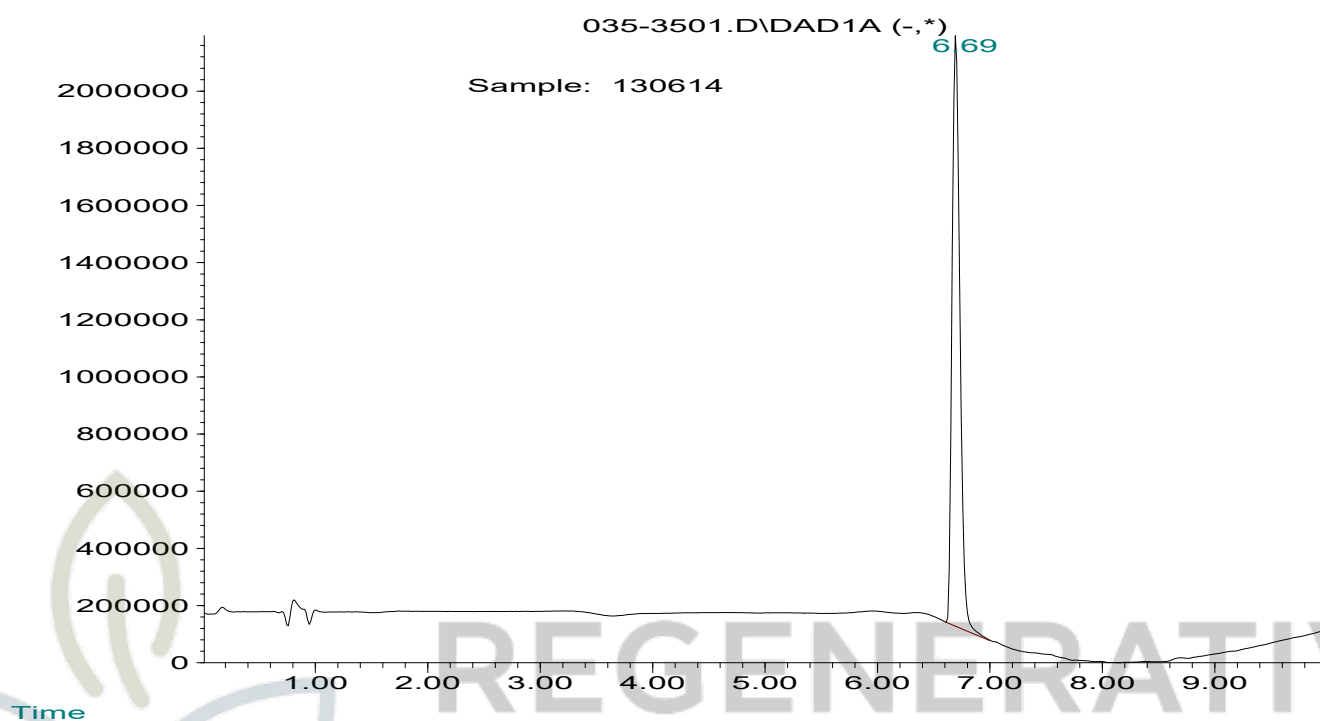

Mass spectrum/Reference Spectrum

