

Randy Cole
Regenerative Research
Denver, CO




Project 135604
Lab # 131351
Date Rec'd 12/18/2025
Report Issued 1/5/2026

Project

Sample Retatrutide 5 mg (RT25-08)

Certificate of Analysis

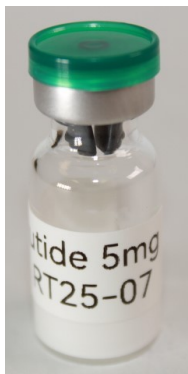

<u>Analyte</u>	<u>Result</u>	<u>LOQ</u>	<u>Units</u>	<u>% of Label</u>	<u>Method</u>	<u>Date</u>	<u>CAS</u>
Peptide Analysis							
Chromatographic purity	>99.95	0.5	%		HPLC-UV/MS	12/29/2025	
Retatrutide	4.65	0.5	mg	93.0	HPLC-UV-MS	12/29/2025	2381089-83-2
Retatrutide	ID Confirmed				HPLC-UV-MS	12/29/2025	
Microbiology							
Endotoxins	ND	1	EU/mL		USP 85	12/31/2025	

The data presented are from the analysis of the sample shown and meet Krause Analytical internal quality assurance criteria unless otherwise flagged.
Methods shown reference current Krause Analytical SOPs
ND - Not detected LOQ - limit of quantification
Copyright © 2025 Krause Analytical LLC. All rights reserved.


Respectfully submitted,

Mark C. Krause
Laboratory Director

**krause analytical**

Chromatogram

Response_

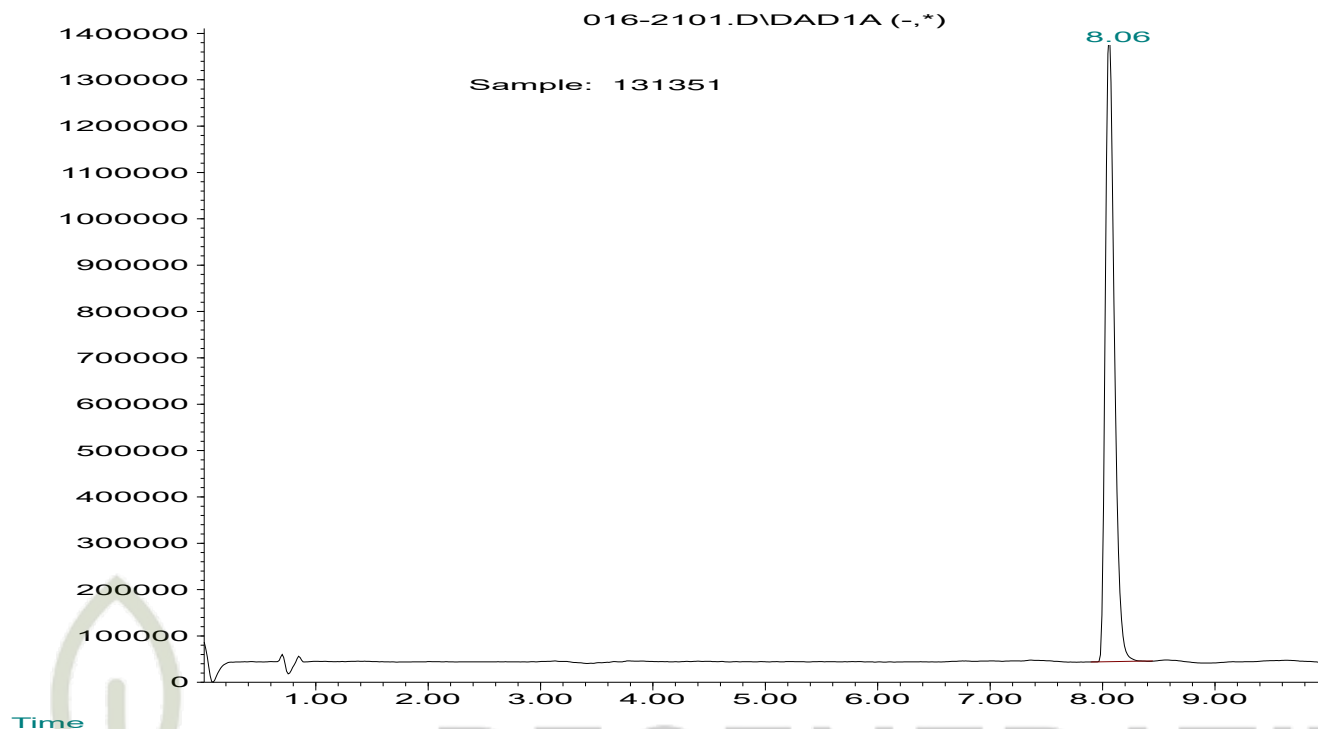

Time

Mass spectrum/Reference Spectrum

