

Randy Cole
Regenerative Research
Denver, CO 80210



Project 135479
Lab # 130211
Date Rec'd 11/12/2025
Report Issued 11/24/2025

Project

Sample Testagen (TT25-01)

Certificate of Analysis

**Analyte****Microbiology**

Endotoxins

Peptide Analysis

Chromatographic purity

Total peptide mass

Testagen

Result**LOQ****Units****Method****Date****% of Label**

ND

1

EU/mL

USP 85

11/21/2025

>99.95

0.5

%

HPLC-UV/MS

11/19/2025

27.1

0.5

mg

HPLC-UV/MS

11/19/2025

108.3

ID Confirmed

HPLC-UV-MS

11/19/2025

The data presented are from the analysis of the sample shown and meet Krause Analytical internal quality assurance criteria unless otherwise flagged.
Methods shown reference current Krause Analytical SOPs
ND - Not detected LOQ - limit of quantification
Copyright © 2025 Krause Analytical LLC. All rights reserved.


Respectfully submitted,

Mark C. Krause
Laboratory Director



Chromatogram

Response_

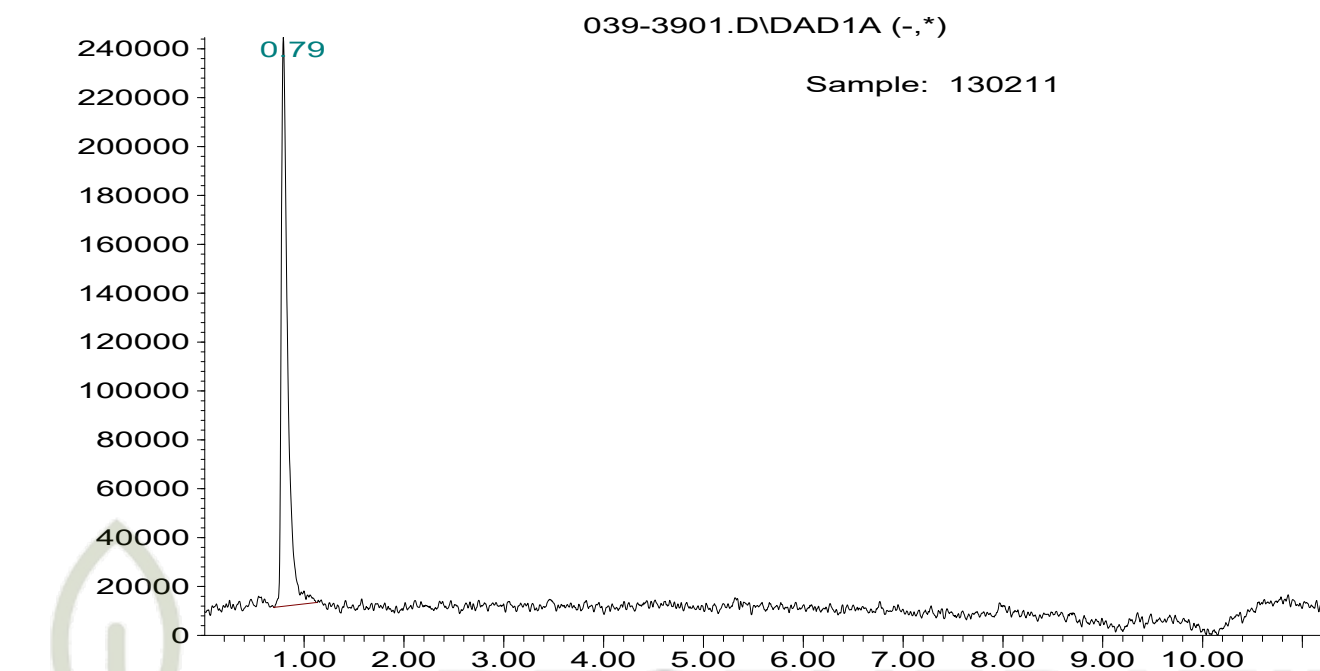

Mass spectrum/Reference Spectrum

