

Randy Cole
Regenerative Research
Denver, CO 80210




Project 135461
Lab # 130122
Date Rec'd 11/6/2025
Report Issued 11/13/2025

Project

Sample AHK-Cu 100 mg (AK25-01)

Certificate of Analysis

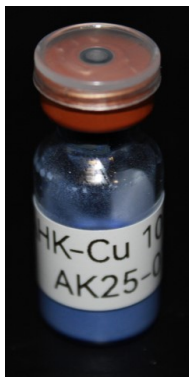

Analyte

Microbiology

Endotoxins

Peptide Analysis

Chromatographic purity

Total peptide mass

AHK-Cu

<u>Result</u>	<u>LOQ</u>	<u>Units</u>	<u>Method</u>	<u>Date</u>	<u>% of Label</u>
ND	1	EU/mL	USP 85	11/10/2025	
99.07	0.5	%	HPLC-UV/MS	11/10/2025	
93.4	0.5	mg	HPLC-UV/MS	11/10/2025	93.4
ID Confirmed			HPLC-UV-MS	11/10/2025	

The data presented are from the analysis of the sample shown and meet Krause Analytical internal quality assurance criteria unless otherwise flagged.
Methods shown reference current Krause Analytical SOPs
ND - Not detected LOQ - limit of quantification
Copyright © 2025 Krause Analytical LLC. All rights reserved.

Respectfully submitted,


Mark C. Krause
Laboratory Director

**krause analytical**

Chromatogram

Response_

003-0301.D\AD1A

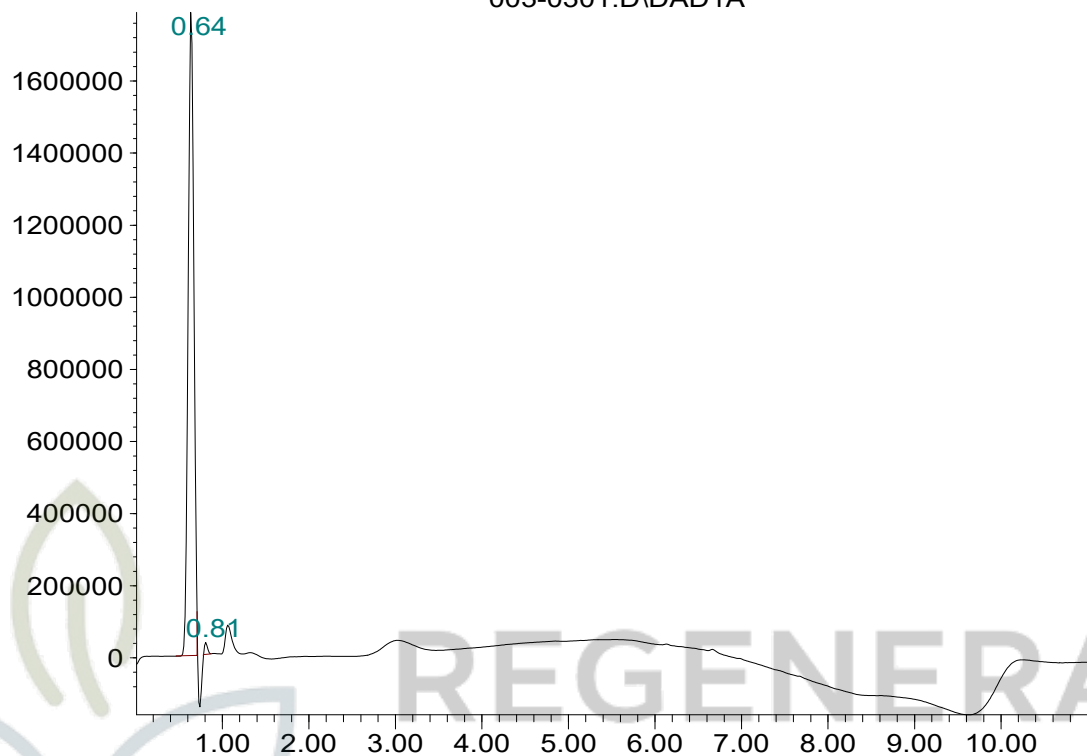

Time

Mass spectrum/Reference Spectrum

