

Regenerative Research
info@regenerativeresearch.co



Project 145123
Lab # 202909
Date Rec'd 3/13/2026
Report Issued 3/30/2026

Certificate of Analysis



Compound Semax
Label Claim 10 mg
Batch/Lot SX26-01

<u>Analyte</u>	<u>Result</u>	<u>Units</u>	<u>LOQ</u>	<u>% of Label</u>	<u>Method</u>	<u>Date</u>	<u>CAS</u>
Peptide Analysis							
Chromatographic purity	>99.9	%	0.5		HPLC-UV/MS	3/25/2026	
Semax	8.18	mg	0.5	81.8	HPLC-UV-MS	3/25/2026	80714-61-0
Mass Spectral Match	ID Confirmed				HPLC-UV-MS	3/25/2026	80714-61-0
Microbiology							
Endotoxins	<0.5	EU/mL	0.5		USP 85	3/30/2026	


The data presented are from the analysis of the sample shown and meet Krause Analytical internal quality assurance criteria unless otherwise flagged.
Methods shown reference current Krause Analytical SOPs
ND - Not detected LOQ - limit of quantification
All values reported on a per vial basis unless otherwise noted
Copyright © 2026 Krause Analytical LLC. All rights reserved.

Respectfully submitted,

Mark C. Krause
Laboratory Director



Chromatogram

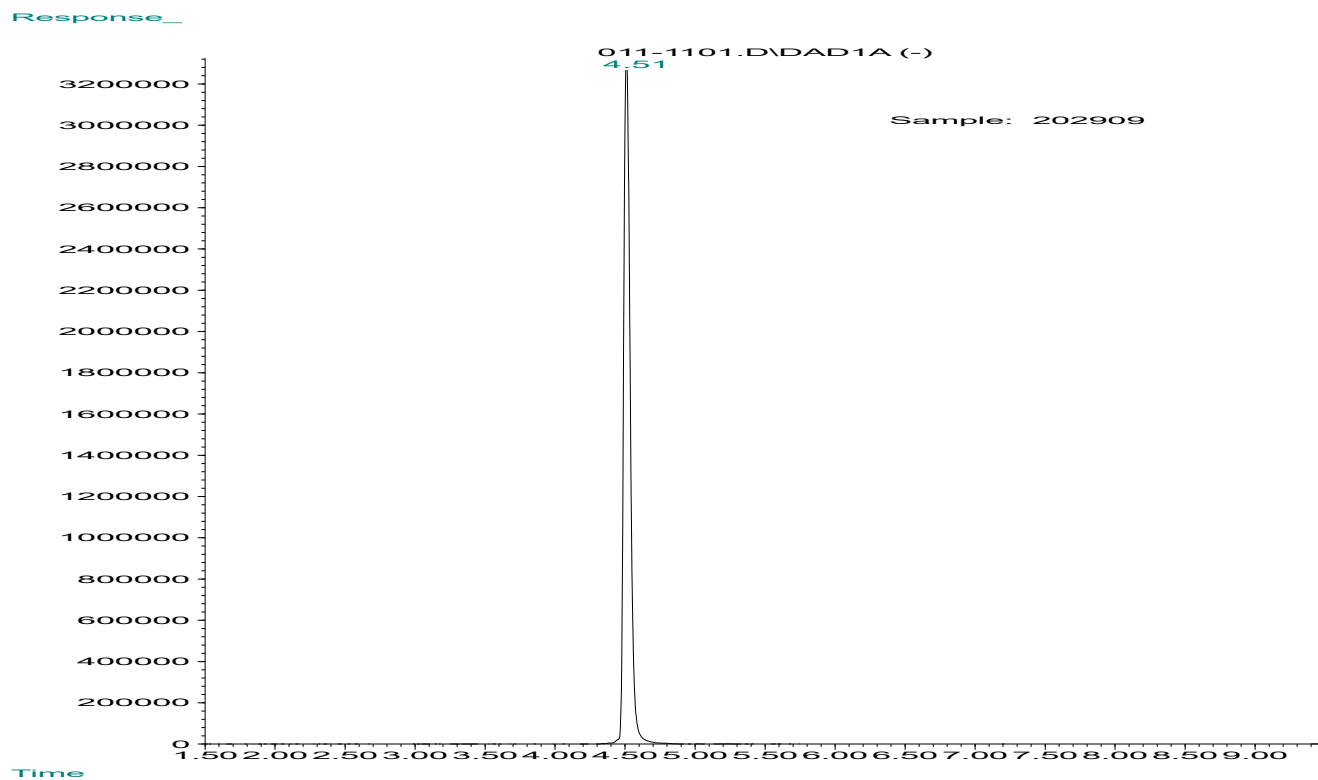

Mass spectrum/Reference Spectrum

